

Version 150604 EN

AdnaTest *OvarianCancer-2 Detect*

RT-PCR Kit for detection of ovarian cancer associated gene expression in enriched tumor cells

For research use only

Manual

REF T-1-539

Contents

Order Information.....	3
Purpose	3
Abbreviations and Symbols	4
Patents and Registered Trademarks	5
Product Description	6
Kit Components	7
Additional Materials Needed	8
Storage	9
Application Information	10
Protocol.....	11
A. Preparation of Dynabeads Oligo(dT) ₂₅	11
B. mRNA Isolation.....	12
C. Reverse Transcription	14
D. Multiplex-PCR (OvarianDetect-2)	16
E. Duplex-PCR (ERCC1-Detect).....	18
F. Fragment Analysis	20
References	25
Troubleshooting	25
Short Manual	26

Order Information

On the website www.adnagen.com the addresses of distributors and information about our products can be found. Our distributors will provide you also with technical support.






Furthermore, the QIAGEN Hannover support team will answer you any questions regarding the *AdnaTests* (support@adnagen.com).

Purpose

AdnaTest OvarianCancer-2 Detect is used for the analysis of ovarian cancer-associated gene expression in immunomagnetically enriched tumor cells by reverse transcription and PCR and is intended for research use only. The specificity of the detection is 90%. In spiking experiments 5 tumor cells in 5 ml of whole blood are detected at a recovery rate of at least 90% and 2 tumor cells in 5 ml of whole blood can be detected at a recovery rate of at least 70%, respectively. In addition, gene expression of ERCC1 (excision repair cross-complementing 1) can also be investigated.

AdnaTest OvarianCancer-2 Select is used for the enrichment of circulating tumor cells from peripheral blood.

Abbreviations and Symbols

<i>AdnaMag-S</i>	Magnetic particle concentrator (-small)
bp	Base pairs
cDNA	Complementary deoxyribonucleic acid
C+	Positive control
C-	Negative control
CA-125	Cancer antigen 125
DNA	Deoxyribonucleic acid
dNTPs	Deoxynucleotide triphosphates
ERCC1	Excision repair cross-complementing 1
GA733-2	Gastrointestinal tumor associated antigen 733-2
mRNA	Messenger ribonucleic acid
Muc-1	Muc-1 gene
PCR	Polymerase chain reaction
RNase	Ribonuclease
rpm	Revolutions per minute
RT	Reverse transcription
	Expiry date
	Storage temperature
	Catalogue number
	Consider instructions for use
	Manufactured by

Patents and Registered Trademarks

This test requires licenses of Hoffmann-La Roche AG, Basel. The purchase of *AdnaTests* does not authorize the user to perform the PCR without license. *Dynabeads®* is a registered trademark of Invitrogen and Life Technologies Corporation. The trademarks *Sensiscript* and *HotStarTaq* are registered by QIAGEN, Hilden. *LabChip* is a US registered trademark of Caliper Technology Corp.

Product Description

AdnaTest OvarianCancer-2 Detect contains Oligo (dT)₂₅-coated beads for the isolation of mRNA from the lysate of pre-enriched tumor cells. Reverse transcription results in cDNA, which is subsequently used as template for tumor cell detection and characterization by Multiplex-PCR. The *PrimerMix Ovarian-2 Detect* allows the amplification of three tumor associated antigens and one control gene. The *PrimerMix ERCC1-Detect* amplifies the excision repair cross-complementing 1 gene (ERCC1) and one control gene. The primers generate fragments of the following sizes:

PrimerMix Ovarian-2 Detect

CA125: 432 bp
GA733-2: 395 bp
Muc-1: 299 bp
Actin: 120 bp (internal PCR control)

PrimerMix ERCC1-Detect

ERCC1: 357 bp
Actin: 120 bp (internal PCR control)

Note: Fragment sizes may vary slightly. Please use the *Positive Control (C+)* 9 and 11 for assignment of the detected signals.

Kit Components

AdnaTest OvarianCancer-2 Detect includes the following components:

Table 1: Kit components

Component	Symbol	T-1-539 (12 tests)
<i>Lysis/Binding Buffer</i>	3	1
<i>Dynabeads Oligo(dT)₂₅</i>	4	1
<i>Buffer A</i>	5	1
<i>Buffer B</i>	6	1
<i>10 mM Tris-HCl</i>	7	1
<i>PrimerMix Ovarian-2 Detect</i>	8	1
<i>Positive Control (C+)</i>	9	1
<i>PrimerMix ERCC1-Detect</i>	10	1
<i>Positive Control ERCC1</i>	11	1

The reagents are sufficient to analyze 6 PCR controls and 12 blood samples.

Additional Materials Needed

Equipment:

- Tube rotator for 1.5 ml tubes
- Magnetic particle concentrator *AdnaMag-S* (QIAGEN Hannover GmbH, cat. no. T-1-800)
- Thermal block or water bath (50 °C)
- Thermocycler with a heated lid and a heating rate of 2 °C/s.
- Analysis system like the Agilent 2100 Bioanalyzer (Agilent Technologies).

Material:

- Sterile, RNase-free thin-wall 0.2 ml PCR-tubes
- Sterile, RNase-free 1.5 ml reaction tubes (e. g. Sarstedt, cat. no. 72.690)
- Pipets and RNase-free pipet tips with aerosol barrier, suitable for pipetting volumes from 1 µl to 200 µl
- Protective gloves

Reagents:

- *Sensiscript* Reverse Transcription Kit (QIAGEN, cat no. 205211, 50 reactions)

Note: The *Sensiscript* Reverse Transcription Kit (cat no. 205211) will suffice for only 25 samples because double volume is required for each reaction.

- Recombinant RNAsin, RNase-inhibitor, 2.500 U (Promega, cat no. N2511)
- *HotStarTaq Master Mix* Kit (QIAGEN, cat no. 203443, 250 U)

Storage

AdnaTest OvarianCancer-2 Detect has to be stored at +4 °C. **However, store the boxes with the *PrimerMixes* and the *Positive Controls* separately at -20 °C.** In order to prevent possible contaminations and repeated temperature changes aliquot the primer mix. All components must not be used beyond the expiry date.

Application Information

- The test must be performed by personnel skilled in molecular biological techniques.
- All components and additional reagents provided by other suppliers have to be stored according to their instructions. Safety advices of the respective manufacturers are valid.
- Wear protective gloves to avoid contamination with DNA, RNA and RNases.



The test has to be performed in the denoted sequence and has to comply with all specifications stated in respect of incubation times and incubation temperatures.

- Perform sample processing incl. reverse transcription and subsequent analysis of amplified PCR products in different rooms, if possible, to avoid cross-contamination.
- **The use of products from other suppliers than suggested may cause inferior results.**
- The safety and hygiene regulations of the laboratory must be respected (e. g. wear lab coats, protective goggles, gloves).

Protocol

Sections A to C describe the isolation of mRNA and reverse transcription, sections D to F deal with Multiplex-/Duplex-PCR and fragment analysis.

A. Preparation of *Dynabeads Oligo(dT)₂₅*

1. Equilibrate *Lysis/Binding Buffer* [3] to room temperature.

Note: Check that the *Lysis/Binding Buffer* contains no precipitate. If any precipitate is observed, equilibrate the buffer to room temperature and mix until it is completely dissolved.

2. Resuspend the *Dynabeads Oligo(dT)₂₅* [4] thoroughly by pipetting before use; do not vortex!
3. Calculate the volume of the beads required for all samples to be processed (20 µl per sample plus 10 %) and transfer the calculated volume into a RNase-free 1.5 ml reaction tube.
4. Place the tube into the *AdnaMag-S*.

Note: The magnet slider of the *AdnaMag-S* can be inserted in two positions. Always insert the slider with forward-facing white plastic film to make sure that the magnets are close to the reaction tubes.

5. After 1 min remove the supernatant with a pipet.

6. Washing
 - a. Remove the magnet slider from the *AdnaMag-S*.
 - b. Add the original volume (step 3) *Lysis/Binding Buffer* [3] and resuspend the beads by repeated pipetting. Resuspend gently to avoid foaming.
 - c. Insert the magnet slider into the *AdnaMag-S*.
 - d. After 1 min remove the supernatant completely.

Repeat once (two washings in total).

7. Remove the tube from the *AdnaMag-S* and resuspend the beads in *Lysis/Binding Buffer* [3] to the original volume (see step 3).

B. mRNA Isolation

Preparation:

1. Equilibrate *Washing Buffer A* [5] and *Washing Buffer B* [6] to room temperature.
2. Place *10 mM Tris-HCl* [7] on ice.
3. Thaw RNase-free water (part of the *Sensiscript Reverse Transcriptase-Kit*, QIAGEN).
4. Adjust a thermal block or water bath to 50 °C.

Processing:

1. Add 20 µl of *Dynabeads Oligo(dT)₂₅* (step A7) to each tube containing cell lysate (*AdnaTest OvarianCancer-2 Select* manual, step B16).
2. Rotate tubes slowly (approx. 5 rpm) for 10 min at room temperature on a device allowing both tilting and rotation.
3. Place the tubes into the *AdnaMag-S* without magnet slider. Swing the *AdnaMag-S* downwards to release beads and liquid captured in the cap.
4. Insert magnet slider and remove the supernatants after 1 min.
5. Washing A
 - a. Remove the magnet slider from the *AdnaMag-S*.
 - b. Add 100 µl Washing *Buffer A* 5 to each tube and resuspend the beads by repeated pipetting. To avoid any loss of beads please rinse lid and tube wall thoroughly.
 - c. Insert the magnet slider into the *AdnaMag-S*.
 - d. After 1 min remove the supernatant completely.

Repeat once (two washings in total).

6. Washing B
 - a. Remove the magnet slider from the *AdnaMag-S*.
 - b. Add 100 µl Washing *Buffer B* 6 to each tube, resuspend the beads by pipetting and transfer into new 1.5 ml reaction tubes.
 - c. Insert the magnet slider into the *AdnaMag-S*.
 - d. After 1 min remove the supernatant completely. This step has to be carried out carefully (watch the pellet) since the beads might be sliding and could be removed by mistake.

Repeat once in the same reaction tubes (two washings in total).

7. Remove the magnet slider from the *AdnaMag-S*.
8. Add 100 µl ice cold 10 mM Tris-HCl [7] to each tube and resuspend the beads by pipetting.
9. Insert the magnet slider into the *AdnaMag-S*.
10. After 1 min remove the supernatants completely.
11. Remove the magnet slider from the *AdnaMag-S*.
12. Resuspend the mRNA/bead-complex in 29.5 µl RNase-free water.
13. Transfer the tubes to a thermal block or water bath and incubate for 5 min at 50 °C.
14. Place the tubes on ice immediately for at least 2 min.
15. Continue immediately (within 5 min) with the reverse transcription (section C).

Do not store the mRNA/bead complex!

C. Reverse Transcription

(*Sensiscript* Reverse Transcriptase Kit, QIAGEN)

1. Thaw 10 x Buffer RT and dNTPs at room temperature, mix by vortexing, centrifuge briefly, and store on ice. Prepare the RT Master Mix on ice.
2. The RT Master Mix is prepared as shown in Table 2 according to the number of samples.

The volume of the Master Mix should be calculated 10 % larger than needed for the total number of reverse transcription reactions. A negative control reaction without addition of mRNA must always be prepared (RT Control).

3. Vortex the RT Master Mix, centrifuge briefly, and pipet 10.5 µl for each reaction into 0.2 ml PCR tubes.
4. Resuspend the mRNA/bead complexes (step B14) carefully with a pipet. Transfer the total volume into the 0.2 ml PCR reaction tube containing the RT Master Mix. Mix thoroughly by repeated pipetting.

Table 2: Reverse Transcription

Component			Volume
RT Master Mix	<i>Sensiscript</i> Reverse Transcriptase Kit (QIAGEN)	10x Buffer RT	4.0 µl
		dNTPs	4.0 µl
		<i>Sensiscript Reverse Transcriptase (SRT)</i>	2.0 µl
	RNase Inhibitor, 40 U/µl (Promega)		0.5 µl
Samples	mRNA/bead-complex or RT Control (RNase-free water)	each ⁽¹⁾ :	29.5 µl
Total volume			40.0 µl

¹⁾ **Note:** As RT Control add 29.5 µl of RNase-free water instead of mRNA/bead-complex. The volume of the mRNA/bead-complex may vary slightly. In any case, use the total volume for reverse transcription!

- cDNA is synthesized in a thermocycler under the following conditions (Table 3).

Table 3: RT program

37 °C	60 min
93 °C	5 min
4 °C	∞

- Place reaction tubes with the cDNA on ice or store at -20 °C for max. 4 weeks.

D. Multiplex-PCR (*Ovarian-2 Detect*)

- Thaw *HotStarTaq Master Mix* (QIAGEN), *Positive Control (C+)* [9], *PrimerMix Ovarian-2 Detect* [8] and RNase-free water, vortex, centrifuge quickly and store on ice.

The PCR Master Mix is prepared as shown in

- Table 4 according to the number of samples.

The volume of the Master Mix should be at least 10 % larger than the requirement calculated from the number of samples. Note that a *Positive Control (C+)* [9], RNase-free water as Negative Control (C-) and the RT Control must always be included.

- For each preparation dispense 42.0 µl of the Master Mix into 0.2 ml PCR reaction tubes. Resuspend the cDNA/bead mix by pipetting and add 8.0 µl of it to each reaction tube.

Note: As Negative Control add 8.0 µl of RNase-free water instead of cDNA.

Table 4: Preparation of the Multiplex-PCR

Component		Volume
PCR Master Mix	HotStarTaq Master Mix	25.0 µl
	RNase-free water	13.0 µl
	<i>PrimerMix Ovarian-2 Detect</i> [8]	4.0 µl
Samples	cDNA or RT Control or Negative Control (RNase-free water) or <i>Positive Control (C+)</i> [9] each:	8.0 µl
Total volume		50.0 µl

A thermocycler is used for the PCR following the program described in Table 5. Run the thermocycler with a ramp of 2 °C/second. The PCR is performed with a total of 37 cycles.

Table 5: PCR program

95 °C	15min] 37 cycles
94 °C	30sec	
58 °C	30sec	
72 °C	30sec	
72 °C	10 min	
4 °C	∞	

E. Duplex-PCR (*ERCC1-Detect*)

1. Thaw *HotStarTaq Master Mix* (QIAGEN), *PrimerMix ERCC1-Detect* [10], *Positive Control ERCC1* [11] and RNase-free water, vortex, centrifuge quickly and store on ice.
2. The PCR Master Mix is prepared as shown in Table 6 according to the number of samples.

The volume of the Master Mix should be at least 10 % larger than the requirement calculated from the number of samples. Note that a *Positive Control ERCC1* [11], RNase-free water as Negative Control (C-) and the RT Control must always be included.

3. For each preparation dispense 42.0 µl of the Master Mix into 0.2 ml PCR reaction tubes. Resuspend the cDNA/bead mix by pipetting and add 8.0 µl of it to each reaction tube.

Note: As Negative Control add 8.0 µl of RNase-free water instead of cDNA.

Table 6: Preparation of the Duplex-PCR

Component		Volume
PCR Master Mix	<i>HotStarTaq Master Mix</i>	25.0 µl
	RNase-free water	13.0 µl
	<i>PrimerMix ERCC1-Detect</i> [10]	4.0 µl
Samples	cDNA or RT Control or Negative Control (RNase-free water) or <i>Positive Control ERCC1</i> [11] each:	8.0 µl
Total volume		50.0 µl

A thermocycler is used for the PCR following the program described in Table 7. Run the thermocycler with a ramp of 2 °C/second. The PCR is performed with a total of 35 cycles.

Table 7: PCR program

95 °C	15min	} 35 cycles
94 °C	30sec	
60 °C	30sec	
72 °C	60sec	
72 °C	10min	
12 °C	∞	

F. Fragment Analysis

Agilent 2100 Bioanalyzer

The analysis with the Agilent 2100 Bioanalyzer (Agilent Technologies) on a DNA 1000 LabChip is recommended. Follow the instructions of the DNA 1000 LabChip manual and make sure that no beads are transferred into the LabChip. Magnetic beads in the gel can cause false results.

Start the Bioanalyzer software "2100 expert". Under "Contexts" select "Instrument", click the button "Assay" next to "Assay selection". Choose "electrophoresis > DNA 1000 Series II.xsy". Prepare the chip and start run. For evaluation of the results set a detection threshold as it is described below:

Under "Contexts" select "Data", choose the tab "Assay Properties". On the right select "Global" and "Normal" from the pull down menu. Choose "Sample Setpoints > Integrator > height threshold (FU)" and set this value to "0" (default value is "20") to detect all signals.

Evaluation (*Ovarian-2 Detect*)

The test is considered positive, if a PCR fragment of at least one tumor associated transcript is clearly detected.

If you are using the Agilent 2100 Bioanalyzer, peaks with a concentration of ≥ 0.2 ng/ μ l are positive (Fig. 1).

The fragment of the control gene actin must show in all patient samples (internal PCR control). An actin signal provides a positive control for a successful cell separation, reverse transcription and Multiplex-PCR. Negative Control and RT Control samples must not show any bands larger than 80 base pairs (primer dimers).

A fragment larger than 1000 bp indicates a contamination with genomic DNA. The separation process was not successful and the results have to be discarded if such a fragment is detected.

Any deviation from the protocol might lead to false negative or false positive results.

In case assistance is needed to interpret the results, please do not hesitate to contact our support team.

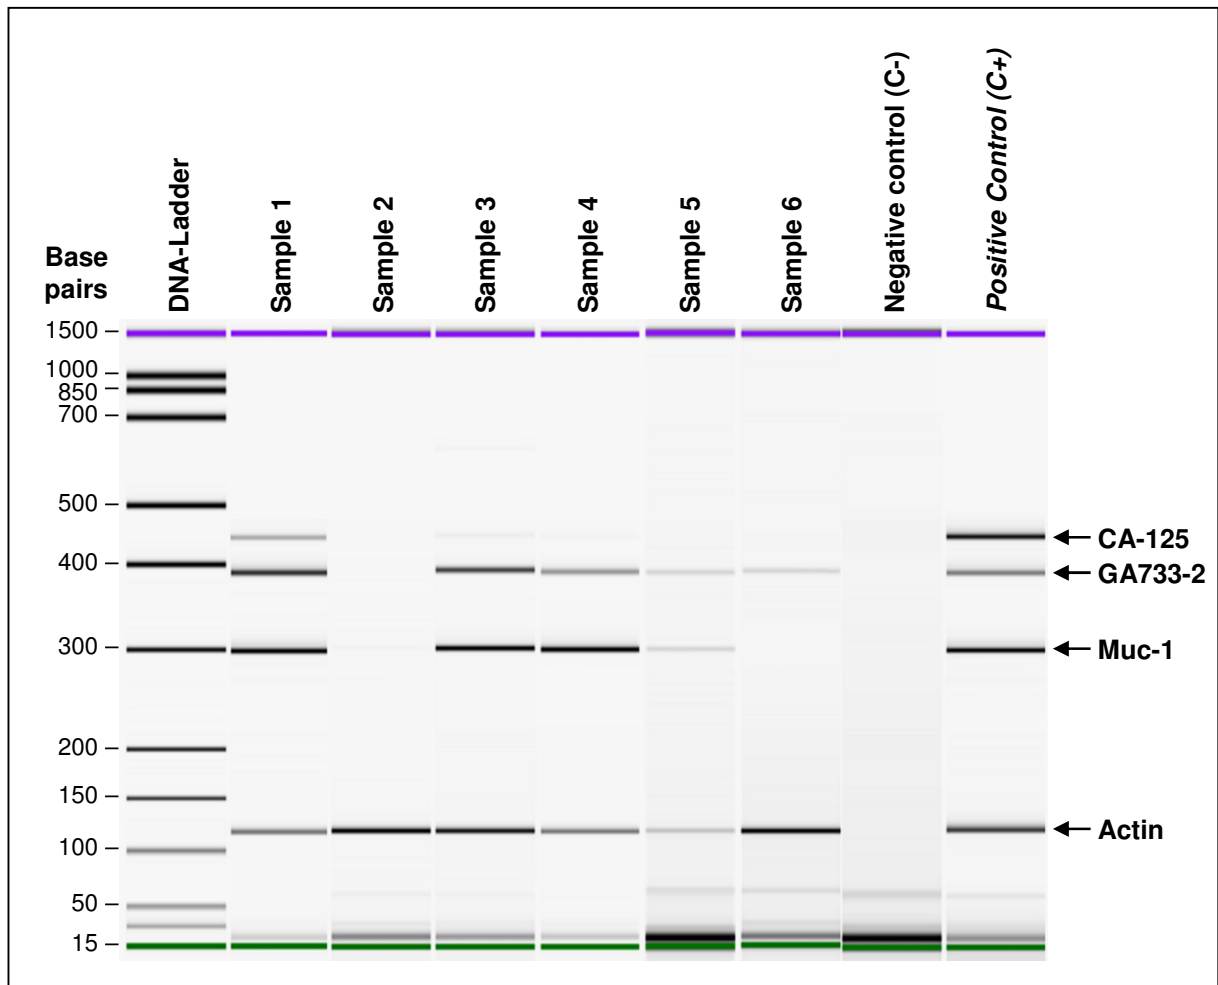


Fig. 1: *AdnaTest OvarianCancer-2 Detect* results of multiplex-PCR samples (*Ovarian-2 Detect*) analyzed with an Agilent 2100 Bioanalyzer

The first lane shows the DNA size standard (DNA-Ladder). Sample 1 is positive for CA-125, GA733-2 and Muc-1, samples 3, 4 and 5 are positive for GA733-2 and Muc-1 and sample 6 is positive for GA733-2. Sample 2 is negative. Actin is detected in samples 1 to 6. The PCR negative (C-) and *Positive Control (C+)* are shown in the last two lanes.

Evaluation (*ERCC1-Detect*)

If you are using the Agilent 2100 Bioanalyzer, peaks with a concentration of ≥ 0.2 ng/ μ l for ERCC1 are positive (Fig. 2).

The fragment of the control gene actin must show in all patient samples (internal PCR control). An actin signal provides a positive control for a successful cell separation, reverse transcription and Duplex-PCR. The Negative Control and the RT Control samples must not show any bands larger than 80 base pairs (primer dimers).

Any deviation from the protocol might lead to false negative or false positive results.

In case assistance is needed to interpret the results, please do not hesitate to contact our support team.

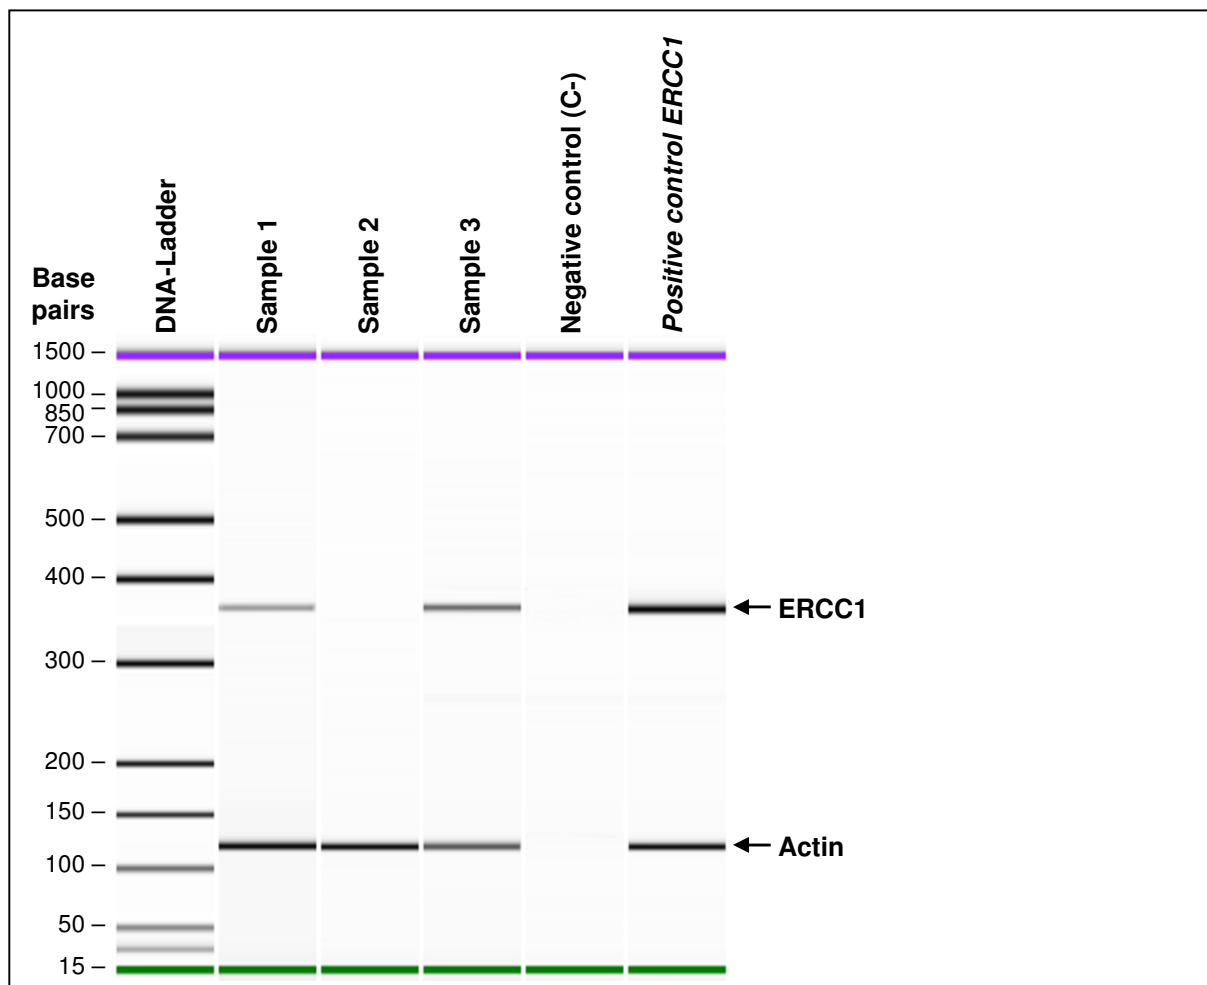


Fig. 2: *AdnaTest OvarianCancer-2 Detect* results of Duplex-PCR samples (*ERCC1-Detect*) analyzed with an Agilent 2100 Bioanalyzer
 The first lane shows the DNA size standard (DNA-Ladder). Samples 1 and 3 are positive for ERCC1. Sample 2 is negative. Actin is detected in samples 1 to 3. The PCR negative (C-) and *Positive control ERCC1* are shown in the last two lanes.

References

For references please refer to our website

<http://www.adnagen.com>

Troubleshooting

A failure of the gene expression analysis may have various reasons. It is essential that all assay steps are always executed precisely according to the manual. In case problems still occur, please go to: www.adnagen.com and download our troubleshooting guide in the product section. You will find practical hints for the test procedure and for the correct interpretation of test results.

Do not hesitate to contact our support team when problems continue to exist.

Short Manual

AdnaTest OvarianCancer-2 Detect

Components	<i>Lysis/Binding Buffer</i>	3
	<i>Oligo (dT)₂₅ Beads</i>	4
	<i>Buffer A</i>	5
	<i>Buffer B</i>	6
	<i>10 mM Tris-HCl</i>	7
	<i>PrimerMix Ovarian-2 Detect</i>	8
	<i>Positive Control (C+)</i>	9
	<i>PrimerMix ERCC1-Detect</i>	10
	<i>Positive Control ERCC1</i>	11
You need	<ul style="list-style-type: none">• 0.2 ml PCR-tubes• 1x 1.5 ml reaction tube per sample• pipets and tips (RNase free) for 1 - 200 µl• <i>Sensiscript</i> RT Kit (QIAGEN)• <i>HotStarTaq Master Mix</i> Kit (QIAGEN)	

Protocol

- Equilibrate [3], [5] and [6] to room temperature and place [7] on ice.
- Wash 20 µl *Oligo(dT)₂₅ Beads* [4] per sample 2x with 20 µl *Lysis/Binding Buffer* [3] per sample.
- Add 20 µl washed *Oligo(dT)₂₅ Beads* [4] to each sample.
- Incubate for 10 min at room temperature under tilting and rotation at approx. 5 rpm.
- Place the reaction tube in *AdnaMag-S* and remove supernatant.
- Wash beads with 2x 100 µl *Buffer A* [5].

Important: To avoid any loss of beads please rinse lid and tube wall thoroughly.

- Resuspend beads in 100 µl *Buffer B* [6] and transfer into a new 1.5 ml tube.
- Wash beads with 1x 100 µl *Buffer B* [6].
- Wash beads with 1x 100 µl *Tris-HCl* [7].
- Resuspend beads in 29.5 µl RNase free water.
- Incubate for 5 min at 50 °C and place on ice for at least 2 min.
- Continue with reverse transcription; see Table 8 and Table 9.

Table 8: Reverse Transcription

Component			Volume
RT Master Mix	<i>Sensiscript</i> Reverse Transcriptase Kit (QIAGEN)	10x Buffer RT	4.0 µl
		dNTPs	4.0 µl
		<i>Sensiscript Reverse Transcriptase (SRT)</i>	2.0 µl
	RNase Inhibitor, 40 U/µl (Promega)		0.5 µl
Samples	mRNA/bead-complex or RT Control (RNase-free water) each ⁽¹⁾ :		29.5 µl
Total volume			40.0 µl

¹⁾ **Note:** As RT Control add 29.5 µl of RNase-free water instead of mRNA/bead-complex. The volume of the mRNA/bead-complex may vary slightly. In any case, use the total volume for reverse transcription!

Table 9: RT program

37 °C	60 min
93 °C	5 min
4 °C	∞

Continue with:

- Multiplex-PCR, Table 10 and Table 11
→ *OvarianDetect-2*
- Duplex-PCR, Table 12 and Table 13
→ *ERCC1-Detect*

or store cDNA at -20 °C for max. 4 weeks

Table 10: Preparation of the Multiplex-PCR

Component		Volume
PCR Master Mix	HotStarTaq Master Mix	25.0 µl
	RNase-free water	13.0 µl
	<i>PrimerMix Ovarian-2 Detect</i> [8]	4.0 µl
Samples	cDNA or RT Control or Negative Control (RNase-free water) or <i>Positive Control (C+)</i> [9] each:	8.0 µl
Total volume		50.0 µl

- The PCR is performed with a total of 37 cycles.

Table 11: PCR program

95 °C	15min] 37 cycles
94 °C	30sec	
58 °C	30sec	
72 °C	30sec	
72 °C	5 min	
4 °C	∞	

- For fragment analysis we recommend the use of an Agilent 2100 Bioanalyzer.

Table 12: Preparation of the Duplex-PCR

Component		Volume
PCR Master Mix	<i>HotStarTaq Master Mix</i>	25.0 µl
	RNase-free water	13.0 µl
	<i>PrimerMix ERCC1-Detect</i> 10	4.0 µl
Samples	cDNA or RT Control or Negative Control (RNase-free water) or <i>Positive Control ERCC1</i> 11 each:	8.0 µl
Total volume		50.0 µl

- The PCR is performed with a total of 35 cycles.

Table 13: PCR program

95 °C	15min	} 35 cycles
94 °C	30sec	
60 °C	30sec	
72 °C	60sec	
72 °C	10min	
12 °C	∞	

- For fragment analysis we recommend the use of an Agilent 2100 Bioanalyzer.



QIAGEN GmbH
QIAGEN Strasse 1
D-40724 Hilden
Germany

For support call

Phone: +49 (0) 511 72 59 50 - 50

Fax: +49 (0) 511 72 59 50 - 40

Email: support@adnagen.com

Internet: www.adnagen.com